

MINIMED™ MOBILE APP | QUICK REFERENCE GUIDE

GETTING STARTED


1 Get started

Check your local Medtronic website to make sure your mobile device is compatible with the MiniMed™ Mobile app.



Download and install the MiniMed™ Mobile app from the Google Play™ or Apple App Store®.

2 Begin setup

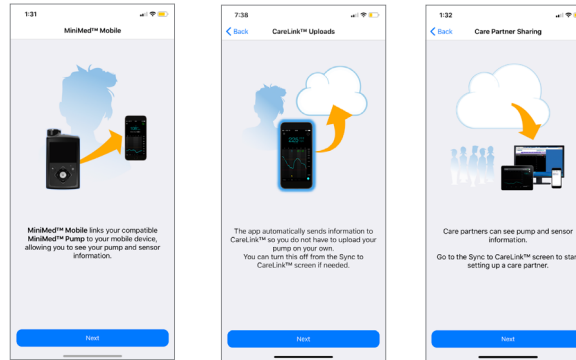


WiFi or mobile data connection is needed for set-up.

View information screens about the app.


NOTE: Care partners can use the CareLink™ Connect app.

3 CareLink™ account

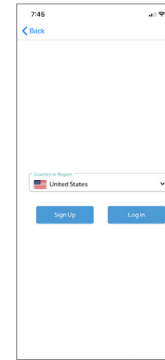

Log in if you already have a CareLink™ account. If not, tap **Sign Up**. Proceed until logged in.

4 Pair your pump to the MiniMed™ Mobile app

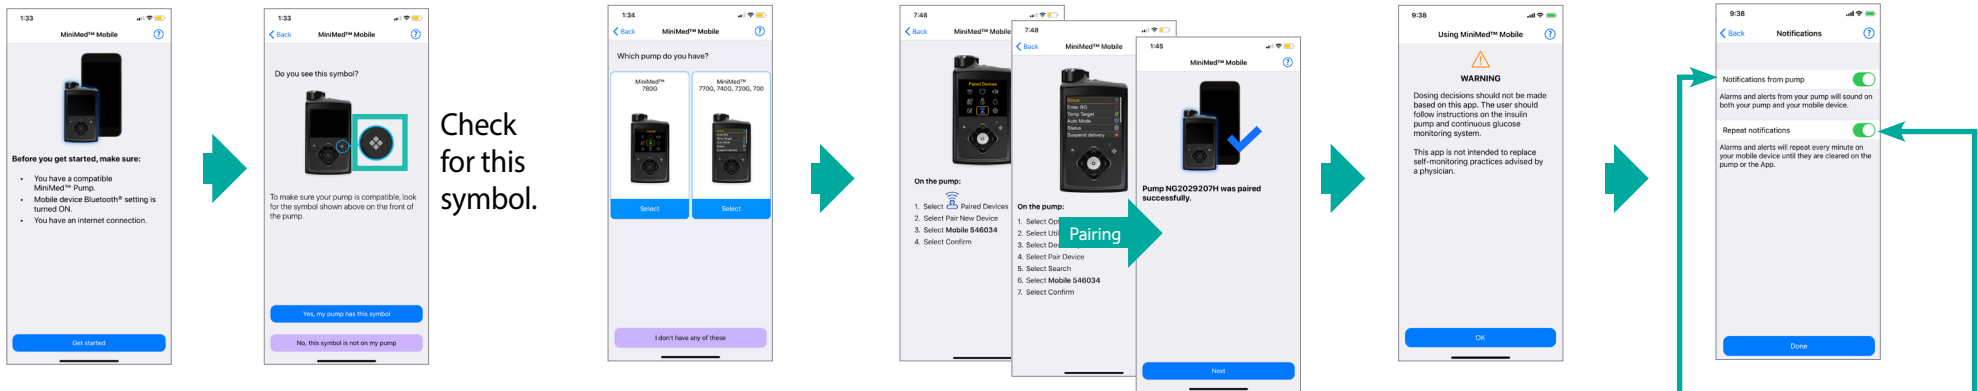

Be sure all three statements are true.

If you do not see this symbol, you cannot use this app. If there is a symbol, continue.

Select the pump that you have. **NOTE:** If asked, you must allow notifications and make data available.


Follow the steps provided to start pairing on the pump. **NOTE:** If asked, tap **Pair** on the app.

Read and agree to the warning information.

Turn on to receive notifications on both pump and app. Turn on to repeat every minute until dismissed on app.

MINIMED™ MOBILE APP | QUICK REFERENCE GUIDE


Home screen

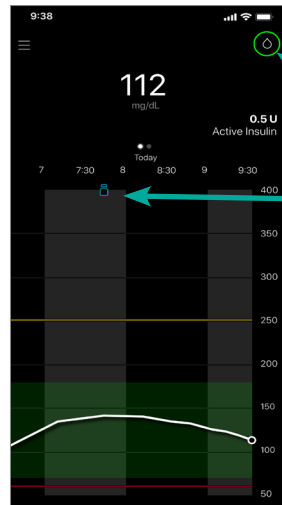

Tap icon for information


Tap icon for event details

Pinch or stretch the graph to change the amount of time displayed.

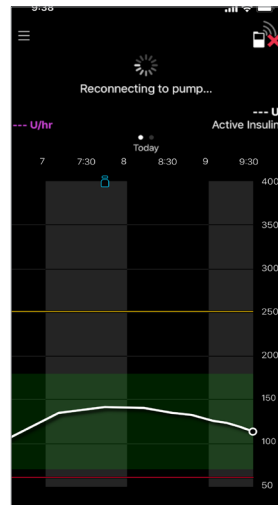


Reconnecting to Pump... appears when the pump and app have been out of range. Allow 60 seconds to reconnect.

Time in range

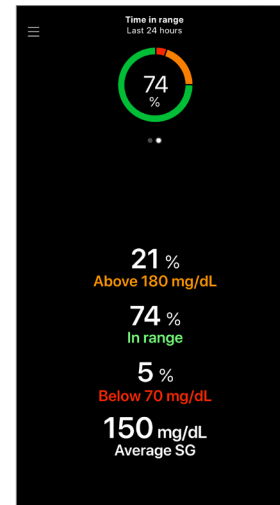

Swipe left on the upper area of the Home screen.

Tap ☰ for menu

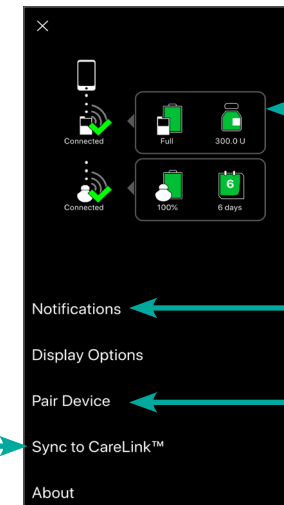

Status: see the status of pump and CGM devices.


Notifications: use to change settings

Pair Device: use if pump and app need re-paired

Sync to CareLink™: Use **Upload Now** to upload current data for reports.

Use **Manage Care Partners** to approve or remove care partners.

Notifications

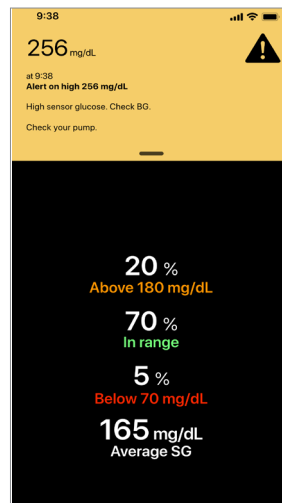

Alarms appear in red

Alerts appear in yellow

Reminders appear in grey

Messages appear in blue



Notifications are not being received on app if this appears at the top of the Home screen.

Tap to turn Notifications on.

NOTE: These must be cleared on the pump even if they are dismissed on the app.

IMPORTANT:

- If a care partner requests to follow you, go to the menu, to **Sync to CareLink** and to **Manage Care Partners** to accept the request.
- For information to be sent to the CareLink™ Connect app, the MiniMed Mobile app must be:
 - within 6 meters (20 feet of the pump)
 - have internet connection
 - be logged into CareLink™ Personal on the app
 - have **Sync to CareLink™** turned on
- If you have questions, tap ☰ and go to **About**. You will find information on many topics there.