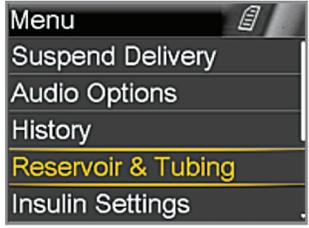
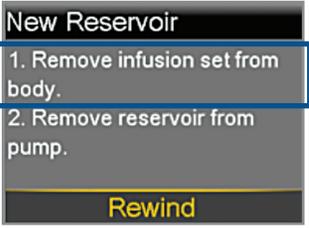


## START HERE:

**1**  Wash your hands. Press .


**2**  Select **Reservoir & Tubing**.

**3**  Select **New Reservoir**.

**4**  Remove the infusion set you have been using by loosening the adhesive and pulling away from body.

**5**  Remove the used reservoir from the pump.

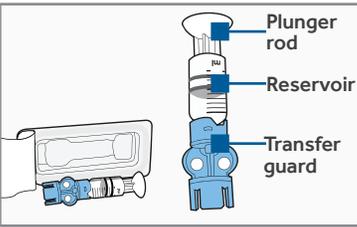



**6**  Select **Rewind**.





**FILL RESERVOIR & CONNECT TO THE INFUSION SET TUBING**

Follow the next steps to fill reservoir with insulin and connect to the infusion set tubing.

**1**  Remove from package. Make sure insulin vial is at room temperature to reduce the risk of air bubbles.

**2**  Pull plunger down to the amount that you plan to fill with insulin.

**3**  Wipe vial with alcohol. Place vial on table. Firmly press the blue transfer guard onto vial.

**4**  Push and hold plunger down.

Continued on next page



**Warning:** Do not use the reservoir or infusion set if any liquid gets on the top of the reservoir or inside the tubing connector. Liquid can temporarily block the vents and may result in the delivery of too little or too much insulin, which can cause hypoglycemia or hyperglycemia.

**5**

Insulin vial  
Plunger

With your thumb still on the plunger, flip over so vial is on top. Release thumb and pull plunger down to fill with insulin.

**6**

Tap the reservoir to move air bubbles to top of reservoir. Push plunger up to move air into vial.

**7**

If needed, pull plunger back down to amount of insulin needed for 2-3 days.

**8**

Reservoir  
Transfer guard

To avoid getting insulin on the top of the reservoir, turn vial over so it is upright. Hold transfer guard and turn reservoir counter-clockwise and remove from transfer guard.

**CONNECT RESERVOIR TO INFUSION SET**

You will place the tubing connector onto the end of the infusion set to the filled reservoir.

**1**

Remove infusion set from package. Remove the paper that holds the tubing together.

**2**

Connector

Gently push the tubing connector onto reservoir. Turn clockwise until locked. You will hear a click.

**3**

If you see air bubbles, tap reservoir to move them to top. Push plunger just a bit to move them into tubing.

**4**

Plunger

Twist plunger counter-clockwise to loosen and remove.

**THE BACKLIGHT MAY HAVE TURNED OFF**

Press any button to turn the screen back on.

Select **Load Reservoir** and unlock pump if necessary.

Select **Next**.


## PLACE RESERVOIR INTO PUMP

Now place the filled reservoir into the reservoir compartment of the pump.

**New Reservoir**  
 3. Place reservoir into pump and lock.  
 DO NOT CONNECT TO BODY.  
 Next

**1** 

Place reservoir into pump.

**2** 

Turn clockwise until you feel reservoir lock into place.

**3** **New Reservoir**  
 3. Place reservoir into pump and lock.  
 DO NOT CONNECT TO BODY.  
 Next

Select **Next**.

## LOAD RESERVOIR AND FILL TUBING

Follow these steps to load the reservoir and fill the tubing.

**1** **Load Reservoir**  
 Select Load and hold until complete.  
 DO NOT CONNECT TO BODY.  
 Load Next

Select **Load** and keep holding .

**2** **Load Reservoir**  
 Complete  
 DO NOT CONNECT TO BODY.  
 Load Next

When you see this screen, select **Next**.

**3** **Fill Tubing**  
 DO NOT CONNECT TO BODY.  
 Hold Fill until drops appear. Then select Next.  
 0.0 u  
 Fill Next

Select **Fill** and keep holding  until you see drops at the end of tubing, then let go.



**Drops at end of tubing**


**4** **Fill Tubing**  
 DO NOT CONNECT TO BODY.  
 Hold Fill until drops appear. Then select Next.  
 11.3 u  
 Fill Next

After you see drops, press  and select **Next**.


## INSERT INFUSION SET

Next, follow the steps to insert the infusion set into your body.

**Fill Cannula?**  
 1. Insert infusion set into body.  
 2. Select Fill to fill cannula or Done if not needed.  
 Fill Done

**1** 

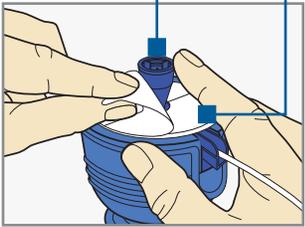
Place blue hub into serter, placing the handle in the tubing slot.


**2** 

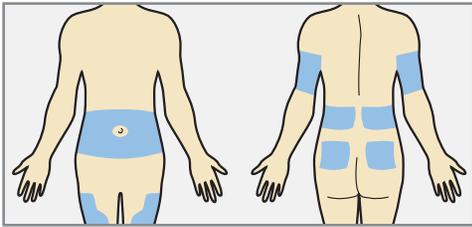
Holding the serter with one hand, gently press infusion set to secure. Be careful not to push all the way into serter. Do not hold or press on the blue button.




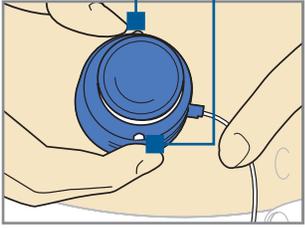
# CHANGING THE QUICK-SET® INFUSION SET MINIMED® 630G INSULIN PUMP

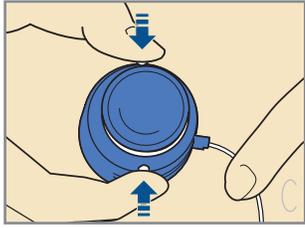
**3** **Needle guard** **Adhesive**  
  
Holding needle guard, pull off the paper that covers the adhesive.

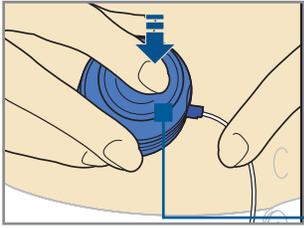
**4** **Blue button**  
  
Pull blue button down until you hear it click.

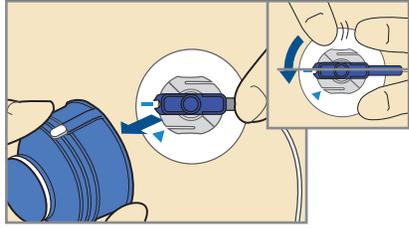
**5**  
  
Choose an insertion site from the shaded areas shown here. Wipe with alcohol or other antiseptic.

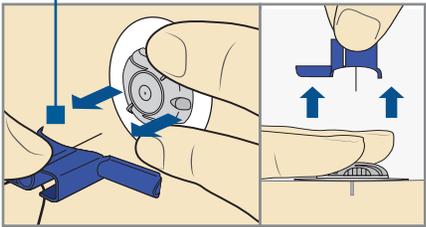
**6** **Needle guard**  
  
Turn to loosen needle guard and pull.


**7** **White buttons**  
  
Hold inserter against cleaned site.

**8**  
  
Press the two white buttons at the same time.

**9** **Blue button**  
  
Press the blue button to unlock.

**10**  
  
Pull inserter away from body. Press adhesive against skin.

**11** **Blue handle**  
  
Hold infusion set. Pull blue handle straight out to remove needle.

**12**  
  
Fold blue handle until locked.

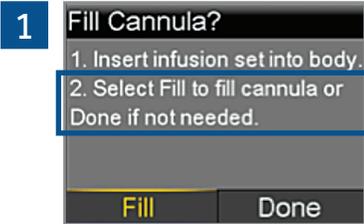
**Dispose blue handle into a sharps container**

Continued on next page



## FILL CANNULA

You will now fill the cannula, the little tube under your skin, with insulin.



Select **Fill**.



Select **Fill amount** and enter:

- 0.300 if using 6mm cannula
- 0.500 if using 9mm cannula

Then press **○**.



**Note:** Your pump will remember the **Fill amount** that you used last. Always verify that the Fill amount is correct.

- If it is correct, press **∨** to **Fill Now** and press **○**.
- If it is incorrect, press **○**. Change to correct amount and press **○**. Select **Fill Now**.



Select **Fill Now**.



The Home screen displays the insulin as it fills the cannula.



**Note:** Select **Stop Filling** if you need to stop, for example, if you notice the **Total** amount is incorrect. This should rarely happen if you have verified the **Fill amount** on the previous screen.

**YOUR  
INFUSION SET  
CHANGE  
IS NOW  
COMPLETE!**